



Patientinstruktion

Klamydia- och gonorrhéprovtagning för personer med vagina


1

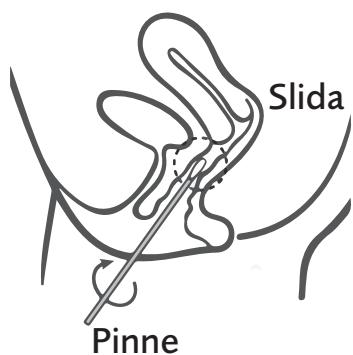

2

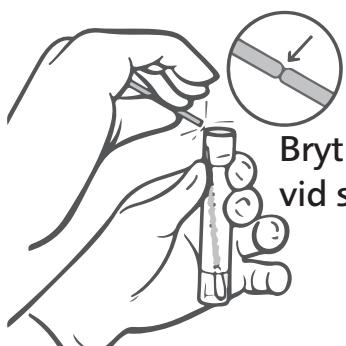


3

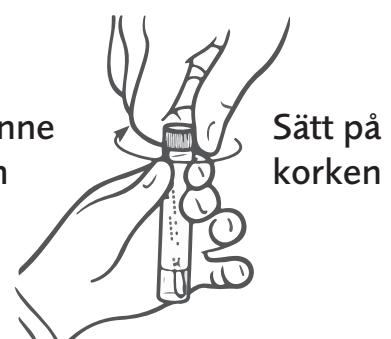


- 1 För bomullspinnen 5 cm in i vaginan.
Rotera pinnen mot vaginans vägg i ungefär 30 sekunder.
- 2 Sätt pinnen i röret med bomullsänden nedåt
– bryt av skaftet vid den markerade skåran på pinnen.
- 3 Skruva på korken på röret ordentligt.
Placera röret i stället eller på anvisad plats.
- 4 Släng resten av provtagningssetet i soppåsen.

Placera röret
i stället


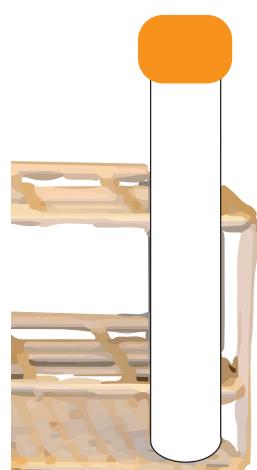


Patientinstruktion

Klamydia- och gonorrhöprovtagning för personer med penis

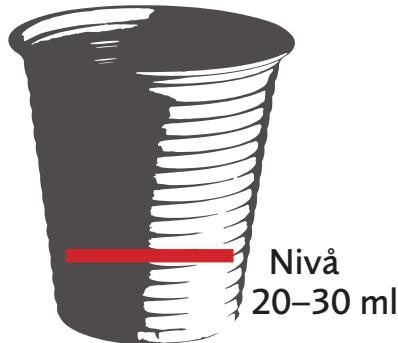



- 1 Det ska ha gått minst en timme sedan du kissade senast.
- 2 Kiss 20–30 ml av den första urinen i muggen (ungefärlig till strecket på bilden).
- 3 Förs över urin till röret med hjälp av plast-pipetten.
OBS! Fyll på med urin tills vätskenivån hamnar i rutan på röret.
- 4 Skruva på korken på röret ordentligt. Placera röret i stället eller på anvisad plats.
- 5 Häll överbliven urin i toaletten. Släng muggen och resten av provtagningssetet i soppåsen.

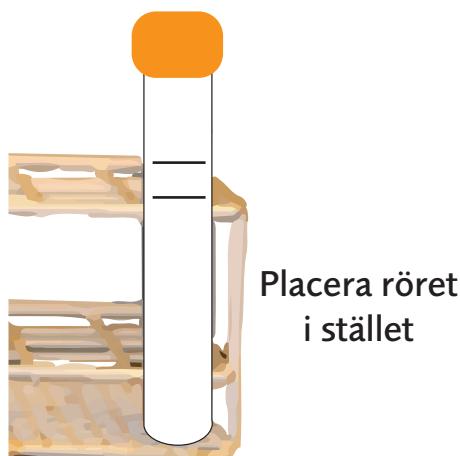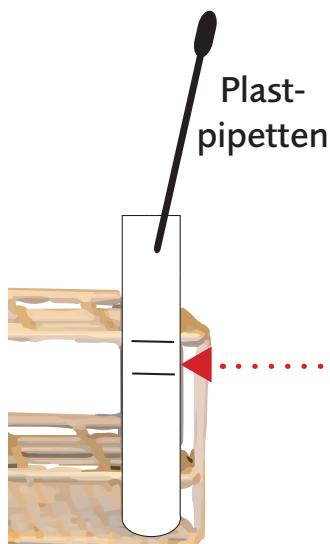


Patientinstruktion

Rektal provtagning klamydia och gonorré -PCR


1

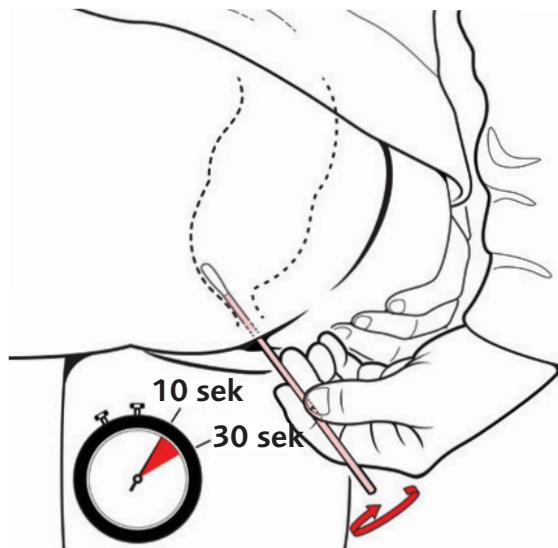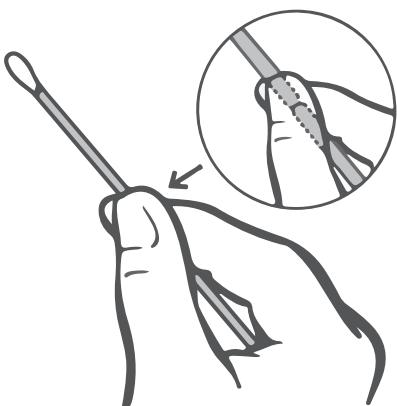

- 1** För in bomullspinnen 2–3 cm i analöppningen, precis förbi slutmuskeln. Rotera pinnen mot slemhinnans vägg i 10–30 sekunder. Om du ser avföring på pinnen ska du ta nytt prov med en ny provtagningspinne.
- 2** Sätt pinnen i provtagningsröret med bomullsänden nedåt – bryt av skaftet vid den markerade skåran på pinnen.
- 3** Skruva på korken på röret ordentligt.
Placera röret på anvisad plats.
- 4** Släng resten av provtagningssetet i soppåsen.


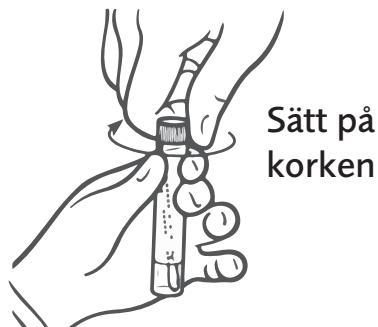


Placera röret
i stället

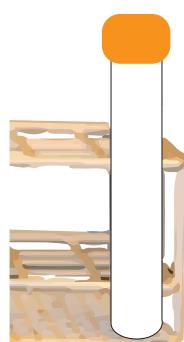


Patient instruction


Anal swab specimen collection for chlamydia and gonorrhoea -PCR

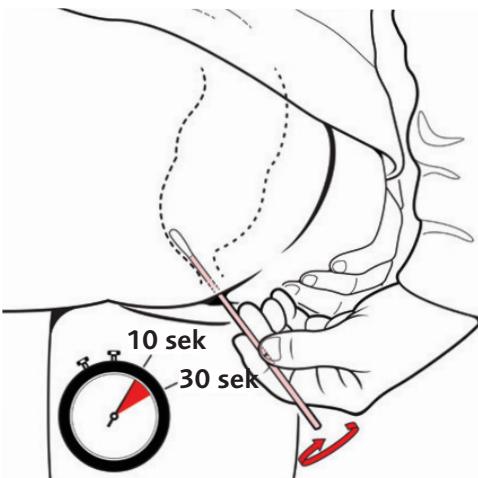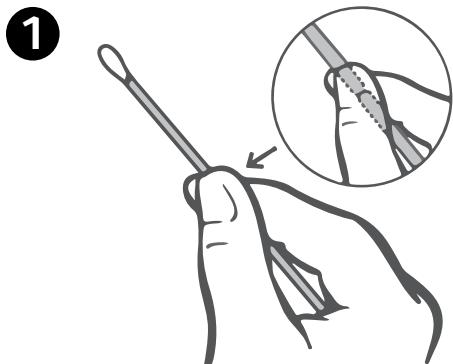


- 1** Insert the cotton swab about 1 inch (2–3 cm) into the anal canal, just passed the anal sphincter muscle. Gently rotate the swab for about 10–30 seconds. If the swab is grossly contaminated with faeces, discard, and repeat the collection with a new swab.
- 2** Place the swab in the test tube with the cotton tip downwards – break the shaft of the swab at the score line.
- 3** Tightly screw the cap onto the tube.
Place the tube in the specified location.
- 4** Dispose of the rest of the sampling kit in the garbage bag.

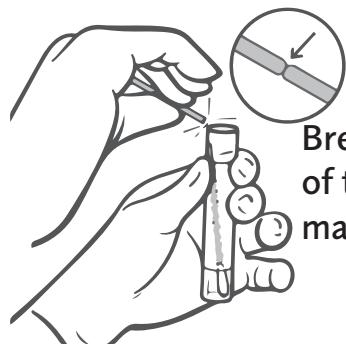

Break the shaft
of the swab at the
marked point

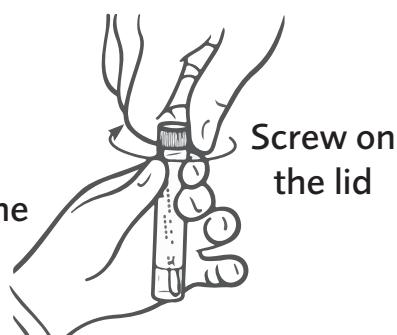

Screw on
the lid

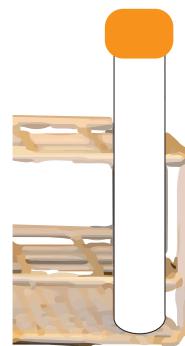


Place the tube in
the specified place


Patient instruction

Chlamydia and gonorrhea testing for a person with vagina


1

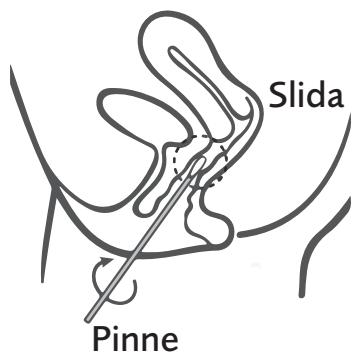

2

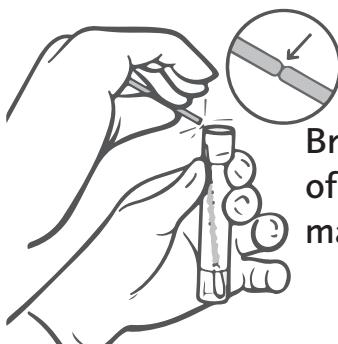

3

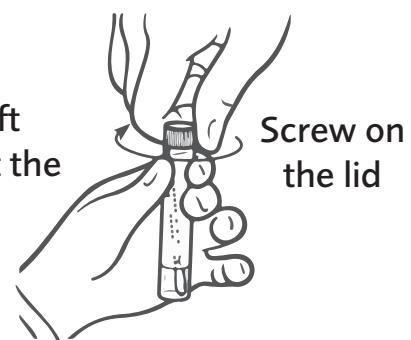


1 Insert the cotton swab 2 inches (5 cm) into the vagina. Rotate the swab against the walls of the vagina for about 30 seconds.

2 Place the swab in the test tube with the cotton tip downwards
- break the shaft of the swab at the score line.

3 Tightly screw the cap onto the tube. Place the tube in the specified location.


Place the tube in the specified place

4 Dispose of the rest of the sampling kit in the garbage bag.

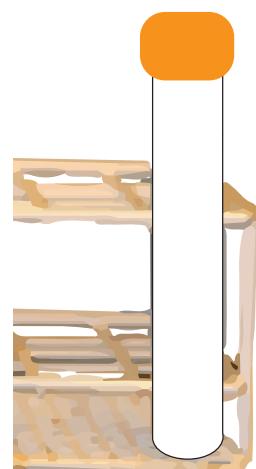


Patient instruction

Chlamydia and gonorrhea testing for a person with penis

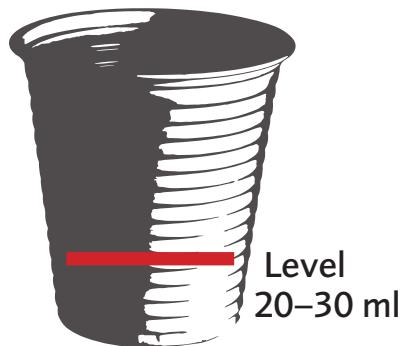

- 1 I must have been at least an hour since you last urinated.
- 2 When urinating, collect the first 20–30 ml in a cup (approximately up to the level of the bar shown in the picture).

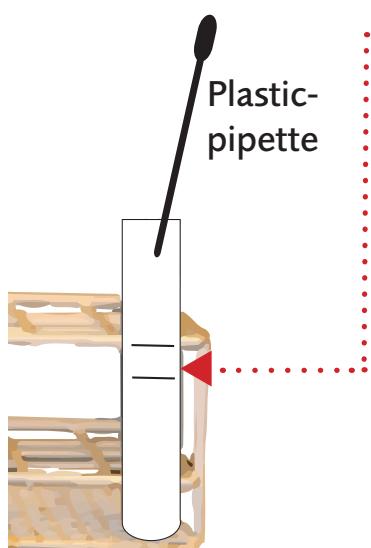

- 3 Transfer the urine to the sample tube using a plastic pipette. **NOTE!** Fill up to the window as shown in the picture.
- 4 Tightly screw the cap onto the tube. Place the tube in the specified location.
- 5 Pour out the remaining urine in the toilet. Dispose of the cup and the rest of the sampling kit in the garbage bag.

